



- Corrects temporal hollowing in patients following a pterional approach to the brain
- Place deep to the temporalis during closure
- Fully porous material for tissue ingrowth
- Implant bends and holds desired shape without heating
- Screws or sutures can be placed in any desired location
- Easy to trim with scissors or scalpel
- Individually packaged, MR Safe, Sterile, 5 Year Shelf Life

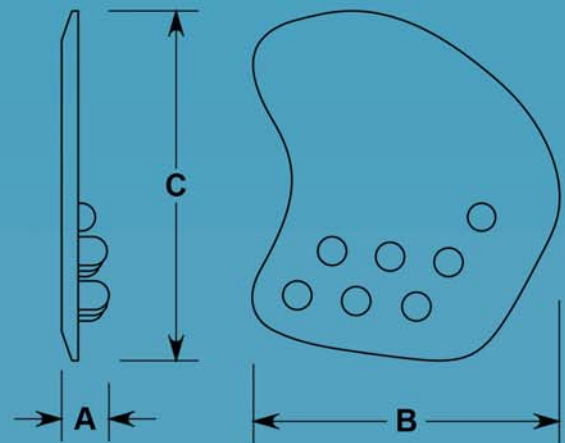

CAT#	Description	A	B	C
4122	Left	6mm	43mm	44mm
4123	Right	6mm	43mm	44mm

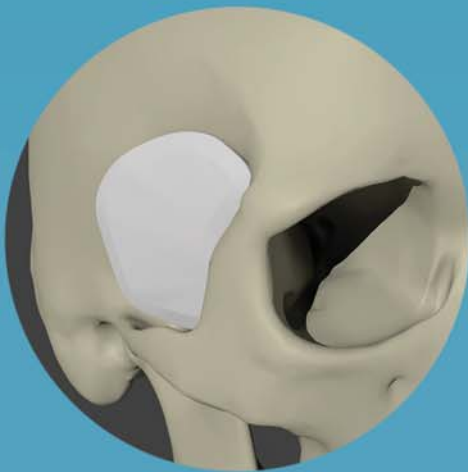